

PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION
International Bureau


INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁵ : A61B 8/12	A1	(11) International Publication Number: WO 95/02995 (43) International Publication Date: 2 February 1995 (02.02.95)
<p>(21) International Application Number: PCT/US94/08352</p> <p>(22) International Filing Date: 20 July 1994 (20.07.94)</p> <p>(30) Priority Data: 08/094,539 20 July 1993 (20.07.93) US</p> <p>(71) Applicant: BIOSENSE, INC. [US/US]; 40 Ramland Road, Orangeburg, NY 10962 (US).</p> <p>(72) Inventor: BEN-HAIM, Shlomo; 29 Stephen Weiss Street, 31080 Haifa (IL).</p> <p>(74) Agent: DIPPERT, William, H.; Cowan, Liebowitz & Latman, 605 Third Avenue, New York, NY 10158 (US).</p>		<p>(81) Designated States: AT, AU, BB, BG, BR, CA, CH, CN, CZ, DE, DK, ES, FI, GB, HU, JP, KP, KR, LK, LU, MG, MN, MW, NL, NO, NZ, PL, PT, RO, RU, SD, SE, SK, UA, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG).</p> <p>Published <i>With international search report.</i> <i>Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i></p>

(54) Title: APPARATUS AND METHOD FOR TREATING CARDIAC ARRHYTHMIAS

(57) Abstract

A method and apparatus for treating cardiac arrhythmias comprising an instrument for mapping ventricular tachycardia, is disclosed. The method is for ablating a portion of an organ or bodily structure of a patient, which comprises obtaining a perspective image of the organ or structure to be mapped; advancing one or more catheters having distal tips to sites adjacent to or within the organ or structure; sensing the location of each catheter's distal tip using a non-ionizing field; at the distal tip of the catheters, sensing local information of the organ or structure; processing the sensed information to create one or more data points; superimposing the data points on the perspective image of the organ or structure; and ablating a portion of the organ or structure. A catheter (51) is introduced into the heart chamber (52) in the body of a patient. An antenna (101) is connected to a receiver (102), and the antennas (103a, 103b, 103c) located at the body surface (57) are transmitting antennas. The transmitter (105) transmits signals to the transmitting antennas (103a, 103b, 103c).

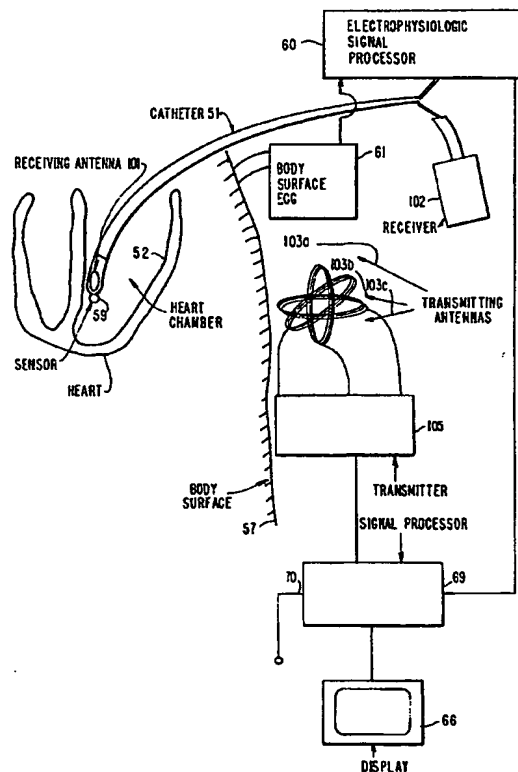

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	GB	United Kingdom	MR	Mauritania
AU	Australia	GE	Georgia	MW	Malawi
BB	Barbados	GN	Guinea	NE	Niger
BE	Belgium	GR	Greece	NL	Netherlands
BF	Burkina Faso	HU	Hungary	NO	Norway
BG	Bulgaria	IE	Ireland	NZ	New Zealand
BJ	Benin	IT	Italy	PL	Poland
BR	Brazil	JP	Japan	PT	Portugal
BY	Belarus	KE	Kenya	RO	Romania
CA	Canada	KG	Kyrgyzstan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SI	Slovenia
CI	Côte d'Ivoire	LI	Liechtenstein	SK	Slovakia
CM	Cameroon	LK	Sri Lanka	SN	Senegal
CN	China	LU	Luxembourg	TD	Chad
CS	Czechoslovakia	LV	Latvia	TG	Togo
CZ	Czech Republic	MC	Monaco	TJ	Tajikistan
DE	Germany	MD	Republic of Moldova	TT	Trinidad and Tobago
DK	Denmark	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	US	United States of America
FI	Finland	MN	Mongolia	UZ	Uzbekistan
FR	France			VN	Viet Nam
GA	Gabon				

APPARATUS AND METHOD FOR TREATING CARDIAC ARRHYTHMIAS

FIELD OF THE INVENTION

5 This invention is directed to an apparatus and method for treating a cardiac arrhythmia such as ventricular tachycardia. More particularly, this invention is directed to an improved apparatus and method whereby there is faster identification of an active site to be ablated.

10 **BACKGROUND OF THE INVENTION**

Cardiac arrhythmias are the leading cause of death in the United States. The most common cardiac arrhythmia is ventricular tachycardia (VT), i.e., very rapid and ineffectual contractions of the heart muscle. VT is the cause death of approximately 300,000 people annually.

15 In the United States, from 34,000 to 94,000 new patients are diagnosed annually with VT. Patients are diagnosed with VT after either (1) surviving a successful resuscitation after an aborted sudden death (currently 20 25-33% of sudden death cases) or (2) syncope, i.e., temporary loss of consciousness caused by insufficient cerebral circulation. The number of VT patients is expected to increase in the future, estimated to range between 61,000 and 121,000 patients annually in five 25 years, as a result of early detection of patients at risk for sudden death by newly developed cardiac tests, advances in cardiopulmonary resuscitation, better medical management of acute myocardial infarction patients, and the demographic shift to a more aged population.

30 Without proper treatment most patients diagnosed with VT do not survive more than two years. The most frequent current medical treatment consists of certain

frequent current medical treatment consists of certain antiarrhythmic drugs or implantation of an automatic implantable cardiac defibrillator (AICD). Drug treatment is associated with an average life span of 3.2 years, a
5 30% chance of debilitating side effects, and an average cost of approximately \$88,000 per patient. In contrast, AICD implantation is associated with a life expectancy of 5.1 years, a 4% chance of fatal complications, and a cost of approximately \$121,000 per patient.

10 In a majority of patients VT originates from a 1 to 2 mm lesion that is located close to the inner surface of the heart chamber. A treatment of VT in use since 1981 comprises a method whereby electrical pathways of the heart are mapped to locate the lesion, i.e., the "active
15 site," and then the active site is physically ablated. In most instances the mapping and ablation are performed while the patient's chest and heart are open. Also, the mapping procedure has been carried out by sequentially moving a hand-held electrical recording probe or catheter
20 over the heart and recording the times of arrival of electrical pulses to specific locations. These processes are long and tedious.

Attempts to destroy, i.e., ablate, the critical lesion are now quite successful, but are currently
25 limited to a small number of patients who can survive a prolonged procedure during which they have to remain in VT for almost intolerable periods of time. The time-consuming part of the treatment is the localization, i.e., identifying the site, of the target lesion to be
30 ablated. Another limitation preventing the wide-spread use of catheter ablation for VT is poor resolution of target localization, which in turn compels the physician to ablate a large area of the patient's heart. The reduction in heart function following such ablation
35 becomes detrimental to most patients with preexisting cardiac damage. However, once the target is correctly

identified, ablation is successful in almost all patients.

5 An improved procedure for treatment of VT must include a faster, more efficient and accurate technique for identifying, or "mapping", the electrical activation sequence of the heart to locate the active site.

10 In electrophysiologic examinations, and in particular in those using invasive techniques, so-called electrical activation mapping is frequently used in combination with an x-ray transillumination. The local electrical activity is sensed at a site within a patient's heart chamber using a steerable catheter, the position of which is assessed by transillumination images in which the heart chamber is not visible. Local
15 electrical activation time, measured as time elapsed from a common reference time event of the cardiac cycle to a fiducial point during the electrical systole, represents the local information needed to construct the activation map data point at a single location. To generate a
20 detailed activation map of the heart, several data points are sampled. The catheter is moved to a different location within the heart chamber and the electrical activation is acquired again, the catheter is repeatedly portrayed in the transillumination images, and its location
25 is determined. Currently catheter location is determined qualitatively or semi-qualitatively by categorizing catheter location to one of several predetermined locations. Furthermore, the transillumination method for locating the catheter does not convey information
30 regarding the heart chamber architecture.

The present technique requires the use of a transillumination means during each of the subsequent catheter employments. This means that if the subsequent catheter locating is achieved by ionizing radiation, the
35 patient and the physician must be subjected to a radiation exposure beyond that which would be required

A catheter which can be located in a patient using an ultrasound transmitter allocated to the catheter is disclosed in U.S. Pat. No. 4,697,595 and in the technical note "Ultrasonically marked catheter, a method for positive echographic catheter position identification." Breyer et al., Medical and Biological Engineering and Computing. May, 1985, pp. 268-271. Also, U.S. Patent No. 5,042,486 discloses a catheter which can be located in a patient using non-ionizing fields and superimposing catheter location on a previously obtained radiological image of a blood vessel. There is no discussion in either of these references as to the acquisition of a local information, particularly with electrical activation of the heart, with the locatable catheter tip and of possible superimposition of this local information acquired in this manner with other images, particularly with a heart chamber image.

20 **OBJECTS OF THE INVENTION**

It is an object of the present invention to provide an alternative method for the permanent portrayal of the catheter during mapping procedures by a method making use of non-ionizing rays, waves or fields, and thus having the advantage of limiting the radiation exposure for the patient and the physician.

It is also an object of the invention to provide a catheter locating means and method that will offer quantitative, high-resolution locating information that once assimilated with the sensed local information would result a high-resolution, detailed map of the information superimposed on the organ architecture.

It is a further object of the present invention to provide a mapping catheter with a locatable sensor at its tip.

These and other objects of the invention will become more apparent from the discussion below.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a schematic block diagram for acquiring a
5 basic image;

FIG. 2 is a schematic block diagram representing a computerized endocardial mapping algorithm;

FIG. 3 is a schematic block diagram representing a computerized pace mapping algorithm;

10 FIG. 4 is a schematic block diagram representing output device configuration of an embodiment of the invention;

FIG. 5 is a schematic block diagram for illustrating the mapping catheter with the sensor at its tip and a
15 locating method in accordance with the principles of the present invention making use of a transmitting antenna at the catheter tip;

FIG. 6 is a schematic block diagram representing use of the invention for pace mapping;

20 FIG. 7 is a schematic block diagram representing the algorithm used to calculate the cross-correlation index while pace-mapping;

FIG. 8 is a diagram representing the catheter used for mapping arrhythmias; and

25 FIGS. 9 and 10 are each a schematic block diagram representing an aspect of the invention.

SUMMARY OF THE INVENTION

30 A trackable mapping/ablation catheter, for use with reference catheters in a field such as an electromagnetic or acoustic field, has (i) a transmitting or receiving antenna for the relevant field within its tip, (ii) a

sensor at its tip for acquiring local information such as electrical potentials, chemical concentration, temperature, and/or pressure, and (iii) an appropriate port for delivering energy to tissue. Receiving or transmitting antennas for the respective field are attached to the patient in which the catheter is disposed. A receiver or transmitter is connected to these antennas and converts the field waves received into electrical locating or image signals. The sensed local information of each site can be portrayed on a display at the respective locations and combined with an image of the structure acquired in a different manner such as by x-ray, NMR, or ultrasound. The resulting information can be used to map the electrical pathways of the heart to determine the situs of a lesion to be ablated.

DETAILED DESCRIPTION OF THE INVENTION

The above objects of the invention are achieved in a method for real-time portrayal of a catheter in the heart chamber, which makes use of a transmitter for electromagnetic or acoustic waves located at the tip of a catheter, these waves being acquired by a receiving antenna attached to the patient and being converted into electrical image signals. The image of the catheter can then be superimposed on a heart chamber image disclosing wall architecture acquired by same or other means of imaging. In an alternative embodiment, the catheter tip may be a receiving antenna, and the externally applied antennas may be transmitting antennas. The sensor in the catheter tip is designed to acquire the information of interest, and the acquisition of local activity at sites located by the tracking methods is used to map the organ under study.

The aforementioned known electromagnetic or acoustic technology permits a simple portrayal of the catheter, because the catheter differs greatly from its environment

(biological tissue) with respect to the interaction of x-rays. The catheter locating technique can be employed with an imaging method and with a corresponding, real-time imaging system which makes use of non-ionizing radiation. The non-x-ray image which portrays the catheter can be combined with an image disclosing heart chamber architecture acquired in an appropriate way. The problem of excess radiation exposure is thus overcome; however, the demands made on the non-ionizing imaging system with respect to its applicability and resolution are rather high.

A further possibility, therefore, is to use the non-ionizing field as part of a locating method, as opposed to an imaging method. Locating methods differ from imaging methods in the following ways: Imaging methods are primarily used to topically correctly portray and resolve a number of subjects or subject points within an image within specific limits. This property is known as the multi-target capability in radar technology and is not present in locating methods. Locating methods operate precisely and unambiguously only in the case wherein a single subject is to be portrayed, i.e., to be located. As an example, the catheter tip is a suitable subject point. The advantage of the locating method is that wave fields can be used wherein the employed wavelength, which is defined by the frequency and phase velocity of the surrounding medium (tissue), can be relatively high, and need not be on the order of magnitude of the locating precision. As is known, range decreases greatly with increasing frequency given non-ionizing waves, such as electromagnetic waves and acoustic waves.

It is thus possible, given the use of a locating method, to make use of relatively long wavelengths, and thus lower frequencies. Moreover, the outlay for signal bandwidth and aperture is much smaller in locating methods than in imaging methods, particularly in view of

the spectral (signal) and spatial (aperture) occupation density. It is sufficient to bring the subject point to be located into interaction with only a few extracorporeal aperture support points, for example, three to five transmitters or receivers, given a few discreet frequencies, for example, three to five frequencies. On the basis of this interaction, ranges or range differences with reference to the subject position and the various aperture supporting points, the combination of which makes an unambiguous and exact positional identification (locating) of the subject point possible, are determined by measuring phase relationships or transit time relationships. The subject point, i.e., the catheter tip, must be marked for this purpose in a suitable manner.

As in conventional pathfinder technology, it is necessary that the catheter image and the heart chamber image be combined with each other in a proper three-dimensional correspondence, and it is also necessary that the heart chamber architecture does not displace or deform during the treatment. To correct for displacement of the heart chamber that occurs during the cardiac cycle the catheter location is sampled at a single fiducial point during the cardiac cycle. To correct for displacement of the heart chamber that may occur because of breathing or patient movement, a set of more than two locatable catheters is placed at specific points in the heart chamber during the mapping procedures. The location of these reference catheters supplies the necessary information for proper three-dimensional correspondence of the heart chamber image and the mapping catheter location.

The above principles can be applied for mapping other structures of the body, for example, of the urinary bladder, brain, or gastrointestinal tract. Dependent upon the examination technique, the catheter may be

replaced by a needle whose tip is the locatable sensor port.

In a broader perspective the invention encompasses four aspects: the first is intended to process locating
5 information; the second processes sensed electrical information; the third integrates previously processed information; and the fourth processes the integrated information to generate a topographical map of the sensed variable. These aspects are described in more detail
10 below.

Catheters will be introduced percutaneously into the heart chambers. Each catheter will be trackable (using the previously described methodology). Preferably three
15 reference catheters will be left in known landmarks, and a fourth catheter will be used as the mapping/ablation catheter. The locations of the three reference catheters will be used to align the location of the heart chamber relative to its location on the "basic image."

20 1. Image and Location Processor

Image acquisition: A method and device to acquire images of the heart chambers from available imaging modalities (e.g., fluoroscopy, echo, MRI, etc.). The
25 image is to be acquired with sufficient projections (e.g., bi-plane fluoroscopy, several longitudinal or transverse cross-sections of echocardiography) to be able to perform 3-dimensional reconstructions of the cardiac chambers' morphology.

Images will be acquired at specific times during the
30 ablation procedure: the basic image will be recorded at the beginning of the procedure to allow determination of the cardiac chamber anatomy and of the positions of reference catheters in the heart. This image will be used thereafter as the basic source of information to
35 describe the heart chamber morphology.

The image and location processor identifies (i) the location of chamber boundaries using the methods of edge enhancement and edge detection, (ii) catheter locations relative to the chamber boundaries, and (iii) the dynamics of chamber morphology as a function of the cardiac cycle.

By analyzing the displacement of the catheter tips during the cardiac cycle the image processor will calculate the regional contractile performance of the heart at a given moment during the mapping/ablation procedure. This information will be used to monitor systolic contractile functions before and after the ablation procedure.

The location processor identifies the locations of catheters. The locations of the reference catheters are used to align the current position of the heart chamber with that of the "basic image." Once current location data is aligned with the "basic image," location of the mapping and ablation catheter is identified and reported.

20

2. Electrophysiologic (EP) Processor

The electrophysiologic signal processor will acquire electrical information from one or more of the following sources:

- 25 A. ECG tracings (by scanning the tracing);
- B. Body surface ECG recordings, either from a 12-lead system (X,Y,Z orthogonal lead system) or from a modified combination of other points on the
- 30 patient's torso; and
- C. Intra-cardiac electrograms, from the ablation/-recording catheter, and/or from a series of fixed catheters within the heart chambers.

At each of the mapping/ablation stages, namely, sinus rhythm mapping, pace mapping and VT mapping, the EP processor will determine the local activation time relative to a common fiducial point in time. The local
5 activation time recorded at each stage will furnish part of the information required to construct the activation map (isochronous map).

The electrophysiologic processor will also perform the following signal processing functions:

10

2.A. Origin Site Determination

Determine the most likely origin site of the patient's arrhythmia based upon the body surface ECG tracings during VT. The most likely VT origin site will
15 be detected by analyzing the axis and bundle morphology of the ECG, and by using the current knowledge of correlation between VT morphology and VT origin site.

2.B. Sinus Rhythm Mapping

20 2.B.1 Delayed Potential Mapping

Using intracardiac electrograms recorded from the mapping catheter tip during sinus rhythm the EP processor will detect and then measure the time of occurrence of delayed diastolic potentials. Detection of late
25 diastolic activity either by (1) ECG signal crossing a threshold value during diastole; or by (2) modelling the electrical activity at a user-defined normal site and then comparing the modelled signal with the actual signal, and estimating the residual from the normal
30 activity; or by (3) using a band pass filter and searching for specific organized high-frequency activities present during diastole; or by (4) using cross-correlation and error function to identify the temporal position of a user-defined delayed potential
35 template. This analysis will be performed on a beat-by-

beat basis, and its results will be available to the next stage of data processing and referred to as the time of delayed potential occurrence.

5 2.C. Pace Mapping

 2.C.1 Correlation Map

 In a "pace mapping mode" the ECG processor will acquire ECG data while the patient's heart is paced by an external source at a rate similar to the patient's
10 arrhythmia cycle length. The ECG data will be acquired from the body surface electrograms, and the signal will be stored as a segment of ECG with a length of several cycles. The signal acquired will then be subjected to automatic comparison with the patient's own VT signal
15 (see Fig. 7). The comparison between arrhythmia morphology and paced morphology will be performed in two stages: First, the phase shift between the template VT signal and the paced ECG morphology would be estimated using minimal error or maximal cross-correlation for two
20 signals. Then, using this phase shift estimated from an index ECG channel, the similarity of the VT and the paced ECG morphology will be measured as the average of the cross-correlation or the square error of the two signals of all channels recorded.

25 This two-stage calculation will be repeated each time using a different ECG channel as the index channel for determining the phase shift.

 At the end of this procedure the minimal error or the maximal cross-correlation found will be reported to
30 the operator as a cross-correlation value (ACI) of this pacing site.

2.C.2 Local Latency

The ECG processor will measure the pacing stimulus to ventricular activation. The earliest ventricular activation will be measured from the earliest zero crossing time of the first derivative signal generated from each of the body surface ECG recordings acquired while pacing. This interval will be reported to the operator and will be later used in the process of judging the suitability of the site for ablation.

10

2.D. VT Mapping

2.D.1 Pre-potential Map

During spontaneous or induced VT the ECG processor will search for a pre-potential present on the mapping/ablation electrode electrogram. The potential will be marked either automatically (by a threshold crossing method, by band pass filtering, or by modelling normal diastolic interval and subtracting the template from the actual diastolic interval recordings) or manually by the user-defined fiducial point on the pre-potential signal. The processor will measure the interval between the time of the pre-potential (PP) signal and that of the earliest ventricular (V) activation as recorded from the body surface tracings, and the interval will be calculated and reported to the user. The ECG processor will report on a beat-by-beat basis the value of the PP-V interval.

15

20

25

2.D.2 Premature Stimuli Local Latency

During VT, when premature extrastimuli will be delivered to the mapping catheter, the ECG processor will detect the time of a single premature signal delivered to the mapping/ablation catheter and the earliest local activation (judged by the presence of non-diastolic activity following a predetermined interval at the

30

35

mapping/ablation catheter and the presence of a different signal morphology shape and value at the body surface electrograms when compared to their value at one cycle length before that event). The presence of electrical activity on the mapping/ablation electrode and the presence of an altered shape of the body surface morphology will be termed as a captured beat. In the presence of a captured beat the ECG processor will calculate the intervals between the stimulus and the preceding earliest ventricular activation (termed V-S) and the interval between the stimulus and the following earliest activation of the ventricle (termed S-V'). The ECG processor will report these intervals to the user after each extrastimulus delivered. Also, the intervals V-S and S-V' will be graphically plotted as a function describing their dependence. The ECG processor will update the plot after each extrastimulus.

2.D.3 Phase Shifting of VT by Premature Stimuli

The ECG processor will identify the effects of the extra-stimulus on the phase shifting of the VT as recorded by body surface electrograms. A user-defined body surfaced channel electrogram of non-paced VT morphology will be used as a template (segment length equal to twice VT cycle length), and the electrogram of the same channel acquired for the same duration following the delivery of an extrastimulus during VT will be used as a test segment. The ECG analyzer will compare the template and the test signal morphologies (using minimal error function or maximal cross correlation) to assure that the VT was not terminated or altered. If VT persists, the ECG analyzer will calculate the phase shift caused by the extrastimulus. Phase shift will be calculated as a part of the VT cycle length needed to be added or subtracted to regularize the VT time series.

2.D.4 VT Termination by Premature Stimuli

The ECG processor will look for a non-capture event following the extrastimulus. In that event the ECG processor will look for alteration in the VT following the extrastimulus delivered. If the VT was terminated (as defined by returning to normal ECG morphology and rate), a note of non-capture termination will be generated by the ECG processor. In case there was no capture but VT morphology did not change, the operator will be notified to change the coupling interval for the coming extrastimuli.

3. Image, Catheter Location and Electrophysiologic Information Integrator

This processor will receive information from the devices described earlier and will attribute the processed electrical information to the specific locations of the heart chamber from which it was recorded. This process will be performed in real time and transferred to the next processor.

Processed electrical information, when combined with its location, generates a map. By use of the previously described variables, the following maps will be generated:

- (1) Spatial location of the endocardium;
- (2) Sinus rhythm activation map (isochronous map);
- (3) Diastolic potential occurrence time isochronal map for sinus rhythm mapping;
- (4) Correlation map for pace mapping;
- (5) Local latency isochronal map during pace mapping;
- (6) Activation time isochronal map during VT; and
- (7) Pre-potential isochronal map during VT mapping.

Also, the sites where VT was terminated by a non-captured premature stimulus will be presented.

At each stage (sinus rhythm mapping, pace mapping and VT mapping) after each data point is acquired, all
5 available information is reassessed for two purposes:
first, to suggest to the operator the next site for data acquisition, and second, to test the available information to propose a site for ablation.

Two algorithms are running simultaneously to perform
10 this procedure:

(1) Mapping guidance algorithm (see Evaluate Activation Map (17) in Fig. 2 and Evaluate Auto-Correlation Map (3a) in Fig. 3). This algorithm uses as an input the available mapped information of a certain
15 variable (e.g., local activation time during sinus rhythm). The algorithm calculates the spatial derivative of the mapped variable (i.e., activation time in this example) and calculates the next best location for adding another data point when the objective function is
20 regularizing the spatial gradients of the mapped variable. For example, this algorithm will suggest that more data points be acquired in areas in which the mapped variable is changing significantly over a short distance.

The location suggested by the algorithm will be
25 presented to the operator as a symbol on the display. The same display already shows the basic image of the heart chamber and the current location of the mapping/ablation catheter. Therefore, the operator will move the mapping/ablation catheter to reach the suggested
30 location for further data acquisition.

This algorithm will become most beneficial during VT mapping, where the available time for data acquisition is limited by the adverse hemodynamic effects of the arrhythmia. Therefore, such an algorithm which examines
35 the available data points of a map in real-time and

immediately suggests the next site for acquisition is greatly needed.

(2) Prognosing likelihood of successful ablation algorithm. This algorithm is a user-defined set of hierarchical rules for evaluating the acquired information. The operator is expected to grade the importance of the specific information acquired in the mapping/ablation procedure, as to its likelihood to identify the correct site for ablation. An example of such an algorithm is described in the following section.

Grading of mapping results suggesting the likelihood of successful ablation at that site (A = highly likely successful and D = least likely successful):

(a) The identification of a typical re-entrant pathway on VT mapping with an identifiable common slow pathway — Grade A;

(b) The identification of a site with over 90% correlation index in the pace map — Grade B;

(c) The identification of a site where VT was terminated with a non-capture premature stimulus — Grade C; and

(d) The identification of pre-potential maps recorded during VT, which are similar to diastolic potential maps recorded during sinus rhythm — Grade D.

25

4. Integrated (Image and Electrical) Processor and Display

The output device will use a computer screen or a holographic imaging unit that will be updated on a beat-by-beat base. The output will include the following information: superimposed on the basic image the position of the catheter will be represented as a symbol on the ventricular wall. The maps will be plotted and overlaid on the same image.

30

The output device at the mode of guided map acquisition would mark on the ventricular wall image the next best place to position the catheter to acquire ECG information based on the results of the previous
5 analysis.

5. Locatable Catheter Mapping and Ablation

Catheters

The catheters used for mapping are critical to the
10 invention. The catheters have a locatable, sensing and/or ablation tip. For locating using electromagnetic fields, locating of the catheter tip is achieved by an antenna disposed at the catheter tip, with an antenna feed guided in or along the catheter. An electrical
15 antenna (dipole) or a magnetic antenna (loop) can be used. The antenna can be operated as a transmission antenna or as a reception antenna, with the extracorporeal antennas located at the skin surface correspondingly functioning as reception antennas or trans-
20 mission antennas. Given multi-path propagation between the catheter tip and the external antennas, the path between the relevant antennas can be calculated by a suitable multi-frequency or broadband technique. It is also possible to employ the locating method using
25 acoustic waves. The problem of the contrast of the biological tissue is significantly less critical when acoustic waves are used than in the electromagnetic embodiment. The problem of multi-path propagation in the case of acoustic waves, however, will be greater for this
30 embodiment because of the lower attenuation offered by the biological tissue. Both problems, however, can be solved as described above in connection with the electromagnetic embodiment.

A ceramic or polymeric piezoelectric element can be
35 used as the antenna at the catheter tip. Due to the high transmission signal amplitudes, operation of the catheter

antenna as a reception antenna is preferred for the case of acoustic locating. Because the transmission paths are reciprocal relative to each other, the locating results are equivalent given reversal of the transmission
5 direction.

The sensor at the catheter tip is constructed with respect to the property to be sensed and the interaction with the locating field waves. For example, a metal electrode for conducting local electrical activity may
10 interact with locating techniques using electromagnetic waves. This problem can be solved in the preferred embodiment by using composite material conductors.

The delivery port at the tip of the catheter is designed with respect to the energy characteristic to be
15 delivered. In the present embodiment the delivery port is the sensing electrode and can function either as an electrode for sensing electrical activity or an antenna to deliver radiofrequency energy to perform ablation of tissue in close contact to the delivery port.

The invention can perhaps be better understood by making reference to the drawings. Fig. 1 is a schematic block diagram for illustrating the acquisition of the basic image. Using a transesophageal echocardiograph (1)
20 in the preferred embodiment, a multiplane image of the heart chambers is acquired prior to the mapping study. The image is acquired only during a fiducial point in time during the cardiac cycle. In the preferred embodiment the image is acquired at end-diastole (2). A three-dimensional image of the heart chambers is reconstructed
25 indicating the endocardial morphology and the location of the reference catheters within the heart chamber (3).

FIG. 2 is a schematic block diagram for illustrating the computerized endocardial activation mapping algorithm (used during sinus rhythm mapping and during ventricular
35 tachycardia mapping). A visible or audible indicator indicates the beginning of a data point acquisition (4).

Data is acquired for each point in the map from two sources. The catheter is in steady and stable contact with the endocardium. The mapping catheter tip is localized (5). The localization of the catheter tip involves the localization of the three reference catheters (7). All locating signals are synchronized to end-diastole (8). The transformation of the three reference catheters relative to their original location in the basic image is calculated (9), and the transformation values in the X,Y, and Z as well as the three orientation movements are applied to the measured location of the mapping/ablation catheter (10), the correction of which yields the location of the mapping/ablation catheter with respect to the basic image (11). Electrical activation acquired with the mapping/ablation catheter tip is analyzed in the electrophysiologic signal processor (6). The local electrogram (12), after being filtered, is analyzed to detect the local activation (14) (by one or more of the techniques for amplitude, slope, and template fitting, or by manual detection by the user). The interval elapsed from previous end-diastole to the present local activation is the local activation time (T, 15). The association of the location of the sensor with the activation time generates a single data point for the activation map (16). The process of data acquisition can be terminated by the user, or can be evaluated by the "evaluate activation map" algorithm (17) that examines the already acquired activation map for the density of information relative to the spatial gradient of activation times. This algorithm can indicate the next preferable site for activation time detection (18). The catheter should be moved by the user to the new site, and the process of mapping continues.

During VT a data point is determined about every 4 to 6 beats. Thus, approximately 15 to 25, typically about 20, data points can be determined each minute.

This factor, in combination with the remainder of the system described herein, permits faster mapping.

FIG. 3 is a schematic block diagram for illustrating the computerized pace mapping algorithm. A visible or audible indicator indicates the beginning of a data point acquisition (20). Data is acquired for each point in the map from two sources. The mapping/ablation catheter is in steady and stable contact with the endocardium, and the mapping/ablation catheter tip is localized (21). The localization of the catheter tip involves the localization of the three reference catheters (22). All locating signals are synchronized to end-diastole (23). The transformation of the three reference catheters relative to their original location in the basic image is calculated (24), and the transformation values in the X, Y, and Z as well as the three orientation movements are applied to the measured location of the mapping catheter (25), the correction of which yields the location of the mapping/ablation catheter with respect to the basic image (26). Body surface ECG acquired is analyzed in the electrophysiologic signal processor (22) according to the pace mapping algorithm. The association of the location of the pacing electrode with the cross-correlation index (ACI, 28) of that site yields a single data point of the pace map (29). The process of data acquisition can be terminated by the user, or can be evaluated by the "evaluate pace map" algorithm (30) that examines the already acquired activation map for the density of information relative to the spatial gradient of cross-correlation index, as well as the presence of circumscribed maxima points in the map. This algorithm can indicate the next preferable site for pacing (31). The catheter should be moved by the user to the new site, pace the heart from that new site and calculate the associated cross-correlation index.

FIG. 4 is a schematic block diagram for illustrating the output device configuration (45) of the present

embodiment. A quasi-static picture of the heart chambers (40) is presented as 3-D reconstruction of a basic image (41) acquired prior to or during the study. Superimposed on the image (40) will be the location of the mapping/ablation catheter (42), locations of the reference catheters (43), and the current and previous information acquired from the mapping study (44). This information may include, when appropriate, the activation times (presented using a color code at each acquisition site) or cross-correlation index for each point in the pace map. Furthermore, the map can represent in the color coding the duration of the local electrograms, the presence of fragmented activity as well as various other variables calculated by the electrophysiologic processor.

FIG. 5 is a schematic block diagram illustrating the instrument while being used for VT mapping. As shown, a catheter (51) is introduced into the heart chamber (52) in the body of a patient. The catheter (51) has an antenna (53) at its tip, which is supplied with energy by a transmitter (54). The transmitting antenna (53) may be, for example, a dipole. The receiver (55) is provided for locating the position of the tip (53). A receiver (55) receives the electromagnetic waves generated by the antenna (53) by means of a plurality of receiving antennae (58a, 58b, and 58c) placed on the body surface (57) of the patient. A sensor (59) placed on the catheter tip receives local electrical activity of the heart chamber muscle. The signals from the sensor electrode (59) are supplied to an electrophysiologic signal processor (60) which calculates the local activation time delay by subtracting the absolute local activation time from the absolute reference time measured from the body surface electrogram (61) of the present heart cycle. A display (66) permits visual portrayal of the local activation times at the location of the catheter tip as described earlier, for example, by superimposition with an ultrasound image showing the heart

chamber architecture. The signals from the receiver (55) and output of electrophysiologic signal processor (60) are supplied to a signal processor (69) which constructs an image of the activation time map.

5 Information regarding the heart chamber architecture is supplied to the signal processor (69) via a separate input (70). The images are superimposed and are portrayed on the display (66). As noted above, the transmitter and receiver may be an ultrasound transmitter
10 or receiver, instead of electromagnetically operating devices.

FIG. 6 is a schematic block diagram illustrating the instrument while being used for pace mapping. The methods for locating catheter tips used in this example
15 are similar to those represented by Fig. 5. Pacing poles (81) are placed on the catheter tip and are connected to a pacemaker (82) source. The pacemaker source activated either by the user or by the electrophysiologic signal processor (84), activates the heart starting at the site
20 of contact of the heart and the pacing poles. Simultaneously acquired ECG (83) is saved and processed in the electrophysiologic signal processor (84). Cross-correlation analysis is carried out in the signal processor (84), and the resulting cross-correlation index (ACI) is
25 transferred to the display unit and associated with the location of the catheter tip to be superimposed on the image of the heart chamber at the appropriate location.

FIG. 7 is a schematic block diagram for illustrating the algorithm used to calculate the cross-correlation
30 index while pace mapping. Body surface ECG data is acquired at two stages. First, during spontaneous or pacing induced VT, and second during pacing the endocardium at different sites. The ECG data acquired during VT are signal averaged, and a template is constructed (T_{ch} , for each channel recorded). During
35 endocardial pacing the ECG data is acquired, and the same

number of beats (N) is acquired to calculate the signal averaged QRS (P_{ch} , for each channel recorded). The algorithm then calculates the phase shift between P_{ch} and T_{ch} , which yields for the first channel the maximal cross-correlation. This time shift is used to shift the remaining channels and calculate for them the cross-correlation. All cross-correlations for all channels are summarized and stored. The algorithm then uses the next channel recorded to calculate the time shift that will cause maximal cross-correlation in this channel. Now this time shift is applied for all cross-correlations between P_{ch} and T_{ch} , and again all cross-correlations are summarized. This procedure is repeated for all channels, and the maximal cross-correlation achieved is used as the value of the cross-correlation of the T_{ch} and the P_{ch} at this site on the endocardium.

FIG. 8 is a schematic diagram illustrating a catheter (90) used for mapping arrhythmias. The distal catheter tip (91) has a conducting material on its outer surface that is the sensing/pacing pole (92) connected to lead (93). In close proximity to pole (92), but separated by insulating material (94), is pole (95), which comprises an annular conducting ring connected to lead (96). The receiver/transmitter antenna (97) of the locating device is placed inside the catheter tip (91), with at least two leads (98) and (99). At least four electrical connections corresponding to leads (93), (96), (98), and (99) exit the catheter: two for the two conducting poles of the sensing/pacing poles and at least two for the locating device antenna.

Although a multitude of catheters (91) could also be used as reference catheters, a catheter (not shown) having only the receiver/transmitter antenna with leads (98, 99) could function suitably. Also, a mapping/ablation catheter (not shown) could be similar in structure to catheter (90) with an additional lumen or

structure or leads to conduct or transmit ablation energy.

An alternative embodiment is shown in FIG. 9, wherein the antenna (101) is a receiving antenna. In this embodiment, the antenna (101) is connected to a receiver (102), and the antennas (103a), (103b) and (103c) located at the body surface (57) are transmitting antennas. The transmitter (105) transmits signals to the transmitting antennas (103a), (103b), and (103c). Operation of the method is otherwise identical to that described in connection with FIG. 5. The embodiment of FIG. 9 can be operated as well using acoustic transmission and reception components instead of electromagnetic transmission and reception components.

FIG. 10 describes a preferred embodiment of a method for proper three-dimensional correspondence of the catheter tip location and the heart chamber image. Three reference locatable catheters (110), (111), (112), as described in the previous sections of this disclosure are placed in fixed positions in the heart, for example, the right ventricular apex, the right atrial appendage, and the pulmonary artery at the level of the pulmonary valve, respectively. The operation method is similar to that described earlier. The location of these three reference catheters is used by the signal processor (69) for proper three-dimensional correspondence of the heart chamber image and the mapping catheter location.

In one embodiment of the invention the mapping procedure can proceed as follows:

1. Insertion of more than two reference catheters (locatable) to fixed positions in the heart.

2. Acquisition of a "basic image" by an imaging modality such as echocardiogram or MR imaging. Image acquired and 3-D reconstructed at end-diastole.

3. Insertion of mapping/ablation catheter (locatable) and positioning of the catheter in the area suspected by VT morphology to include the "active site."
4. Sinus rhythm mapping to construct sinus rhythm activation maps and diastolic potential isochronal maps.
5. Pace Mapping:
 - (a) Construction of ACI map.
 - (b) Construction of local latency map.
6. VT Mapping
 - 10 (a) Activation mapping: Construction of activation map during VT.
 - (b) Pre-potential isochronal map.
 - (c) Extrastimuli pacing during VT.
 7. Ablation
 - 15 (a) Detection of optimal location of ablation from the data acquired with the above mapping.
 - (b) Positioning the mapping/ablation catheter on top of the endocardial site;
 - (c) Measuring systolic contractile function at that site;
 - 20 (d) Delivering ablative energy to the preferred site;
 - (e) Repeating step (c)
- 25 As can be appreciated, the overall mapping procedure to determine an "active site" is complex and includes several stages, none of which is mandatory. Dependent upon the results obtained in each stage, mapping may continue.
- 30 Specific aspects of the procedure can be performed in the following sequence:
 - Through a percutaneous venous access three reference catheters are introduced into the heart and/or the large

vessels. The three reference catheters are positioned so that the respective distal tips are at least 2 cm, preferably 4 to 8 cm, apart. Next, A 3-D image of the chamber of interest is reconstructed using, for example, transesophageal ultrasonography. Then, the locations of the distal tips of the reference catheters are marked.

Through another vascular access port a mapping/ablation catheter is introduced to the area of interest, and then the location of its distal tip as well as the sensed electrical activity are recorded. The location of the mapping/ablation catheter is measured relative to the location of the reference catheters.

In a modified embodiment of this invention the map previously described can be superimposed on the mapped organ image.

Once the operator identified an active site, the mapping/ablation catheter is positioned so that the active site can be ablated. The ablation is performed by radiofrequency energy. Other known methods could be used instead (e.g., laser, cryotherapy, microwave, etc.).

Although modifications and changes may be suggested by those skilled in the art, it is the intention of the inventor to embody within the patent warranted hereon all changes and modifications as reasonably and properly come within the scope of their contribution to the art.

I CLAIM:

1. A method for mapping an organ or bodily structure of a patient, which comprises the steps of:

- 5 (a) obtaining a perspective image of the organ or structure to be mapped;
- (b) advancing one or more catheters having distal tips to sites adjacent or within the organ or structure;
- (c) sensing the location of each catheter distal tip using a non-ionizing field;
- 10 (d) processing the sensed information from step (c) to create one or more data points; and
- (e) superimposing said one or more data points from step (d) on the perspective image of the organ or structure.

15 2. A method for mapping an organ or bodily structure of a patient, which comprises the steps of:

- (a) obtaining a perspective image of the organ or structure to be mapped;
- (b) advancing one or more catheters having distal tips to sites adjacent or within the organ or structure;
- 20 (c) sensing the location of each catheter distal tip using a non-ionizing field;
- (d) at the distal tip of one or more catheters sensing local information of the organ or structure;
- 25 (e) processing the sensed information from steps (c) and (d) to create one or more data points; and
- (f) superimposing said one or more data points from step (e) on the perspective image of the organ or structure.
- 30 3. The method of Claim 2, wherein steps (d) and (e) are repeated a number of times sufficient to create a map to be superimposed in step (f).

4. A method for mapping an organ or bodily structure of a patient, which comprises the steps of:

(a) advancing one or more catheters to sites adjacent to or within an organ or bodily structure;

5 (b) sensing the location of each catheter distal tip using a non-ionizing field;

(c) at the distal tip of one or more catheters sensing local information of the organ or structure;

(d) processing the sensed information from steps
10 (b) and (c) to create one or more data points; and

(e) transmitting said one or more data points to a receiving means.

5. The method of Claim 4, wherein steps (c) and (d) are repeated a number of times sufficient to create a
15 map to be transmitted in step (e).

6. The method of Claim 4, wherein in step (e) said one or more data points are projected onto an image receiving means.

7. A method for mapping an organ or bodily
20 structure of a patient, which comprises the steps of:

(a) advancing one or more catheters to sites adjacent to or within an organ or bodily structure;

(b) sensing the location of each catheter distal tip using a non-ionizing field;

25 (c) creating one or more data points from the sensed information; and

(d) transmitting said one or more data points to a receiving means.

8. The method of Claim 7, wherein steps (b) and
30 (c) are repeated a number of times sufficient to create a map to be transmitted in step (d).

9. The method of Claim 7, wherein in step (d) said one or more data points are projected onto an image receiving means.

10. The method of Claim 1, 2, 4, or 7 wherein the
5 organ is the heart.

11. The method of Claim 10, wherein the local information sensed is the heart's electrical activity.

12. The method of Claim 1, 2, 4, or 7 wherein four
10 catheters are advanced, three of which are reference catheters and the fourth of which is a mapping/ablation catheter.

13. A method for ablating a portion of an organ or bodily structure of a patient, which comprises the steps of:

15 (a) obtaining a perspective image of the organ or structure to be mapped;

(b) advancing one or more catheters having distal tips to sites adjacent to or within the organ or structure, at least one of said catheters having ablation
20 ability;

(c) sensing the location of each catheter's distal tip using a non-ionizing field;

(d) at the distal tip of one or more catheters sensing local information of the organ or structure;

25 (e) processing the sensed information from steps (c) and (d) to create one or more data points;

(f) superimposing said one or more data points from step (e) on the perspective image of the organ or structure; and

30 (g) ablating a portion of the organ or structure.

14. The method of Claim 13, wherein steps (d) and (e) are repeated a number of times sufficient to create a map to be superimposed in step (f).

15. A method for ablating a portion of an organ or bodily structure of a patient, which comprises the steps of:

- 5 (a) advancing one or more catheters to sites adjacent to or within an organ or bodily structure, at least one of said catheters having ablation ability;
- (b) sensing the location of each catheter's distal tip using a non-ionizing field;
- (c) at the distal tip of one or more catheters
10 sensing local information of the organ or structure;
- (d) processing the sensed information from steps (b) and (c) to create one or more data points;
- (e) transmitting said one or more data points to a receiving means; and
- 15 (f) ablating a portion of the organ or structure.

16. The method of Claim 15, wherein steps (c) and (d) are repeated a number of times sufficient to create a map to be transmitted in step (e).

17. The method of Claim 15, wherein in step (e)
20 said one or more data points are projected onto an imaging receiving means.

18. The method of Claim 13 or 15, wherein the organ is the heart.

19. The method of Claim 18, wherein the local
25 information sensed is the heart's electrical activity.

20. The method of Claim 19, wherein the ablation is carried out to treat ventricular tachycardia, ventricular fibrillation, atrial tachycardia, atrial fibrillation, or atrial flutter.

21. The method of Claim 13 or 15, wherein four
30 catheters are advanced, three of which are reference catheters and the fourth of which is a mapping/ablation catheter.

22. A method for treating ventricular tachycardia, which comprises the steps of:

(a) obtaining a perspective image of a patient's heart;

5 (b) advancing two or more reference catheters and one mapping/ablation catheter, all of which catheters have distal tips, to sites within the heart;

(c) sensing the location of each catheter's distal tip using a non-ionizing field;

10 (d) at the distal tip of the mapping/ablation catheter sensing information concerning the heart's electrical activity;

(e) processing the information sensed in steps (c) and (d) to create one or more data points;

15 (f) superimposing said one or more data points from step (e) on the perspective image of the heart to create a representation of the heart's electrical pathway;

(g) studying said representation to determine an active site for ablation; and

20 (h) ablating a portion of the inner surface of the ventricle.

23. The method of Claim 22, wherein steps (d) and (e) are repeated a number of times sufficient to create a map to be superimposed in step (f).

25 24. A method for treating cardiac arrhythmias, which comprises the steps of:

(a) advancing one or more reference catheters and one or more mapping/ablation catheters, all of which have distal tips, to sites within a patient's heart;

30 (b) sensing the location of each catheter distal tip using a non-ionizing field;

(c) at the distal tip of the mapping/ablation catheter sensing information concerning the heart's electrical activity;

(d) processing the information sensed in steps (b) and (c) to create one or more data points;

(e) transmitting said one or more data points to a receiving means; and

(f) ablating a portion of the inner surface of the ventricle.

10 25. The method of Claim 24, wherein steps (c) and (d) are repeated a number of times sufficient to create a map to be projected in step (e).

26. The method of Claim 24, wherein in step (e) said one or more data points are projected onto an image receiving means.

27. A method of prognosing the likelihood of successful treatment of cardiac arrhythmia at a specific site in a patient's heart, said method comprising calculating the similarity of a patient's body electrogram morphology during arrhythmia to the patient's body surface electrogram during pacing in a plurality of sites on the endocardium of the patient's heart.

28. The method of Claim 27, wherein said method is a closed-heart method.

25 29. The method of Claim 27, wherein said calculating comprises the steps of:

(a) determining the similarity of the patient's body surface electrogram morphology during arrhythmia to the body surface electrogram morphology during pacing from a plurality of sites, and

(b) creating a map of corresponding similarity discriminant of said locations of endocardium.

30. The method of Claim 27, wherein said calculating is carried out by determining the correlation between an ECG of the patient during arrhythmia and pacing in a plurality of sites on the endocardium.

5 31. The method of Claim 27, 29, or 30, wherein ventricular tachycardia or ventricular fibrillation is treated.

10 32. A method for automatic guidance of an operator-performed mapping procedure, said method comprising the steps of:

(a) recording the values of a mapped variable at a plurality of locations to prepare a map; and

(b) evaluating the resulting map to identify the optimal site for further acquisition of information.

15 33. The method of Claim 32, wherein said method for evaluating the resulting map comprises calculating the spatial gradients of the mapped variable.

34. The method of Claim 32, wherein the mapped variable is local activation time.

20 35. The method of Claim 32, wherein the mapped variable is derived by comparing electrogram morphology acquired in a plurality of sites.

25 36. A method for automatic guiding of a mapping procedure in a patient, said method comprising the steps of:

(a) detecting a preferred location for future data acquisition, and

(b) presenting the current site of a mapping catheter and the proposed location for future ablation.

30 37. A method for prognosing the likelihood of successful treatment of cardiac arrhythmia of a patient, said method comprising mapping the electrical activity of the endocardium in the heart of said patient.

38. The method of Claim 37, wherein said electrical activity is mapped in a closed-heart method.

39. The method of Claim 37, wherein the electrical activity is delayed diastolic potential.

5 40. The method of Claim 37, wherein mapping means acquires location and sends local information at the same heart cycle.

41. The method of Claim 37, wherein the electrical activity is pre-potential.

10 42. A method for automatic location of a catheter in a patient's heart using a plurality of fixed, reference catheters, said method comprising the steps of:



 (a) locating a plurality of reference catheters;
 (b) locating a mapping catheter relative to the
15 location of the reference catheter; and

 (c) determining the mapping catheter location after accounting for movement of the reference catheters.

43. The method of Claim 42, wherein said method is a closed-heart method.

20 44. The method of Claim 42, which comprises the steps of:

 (a) advancing one or more catheters to sites adjacent to or within an organ or bodily structure;
 (b) sensing the location of each catheter distal
25 tip using a non-ionizing field;
 (c) processing the sensed information from step (b) to create one or more data points; and
 (e) transmitting said one or more data points to a receiving means.

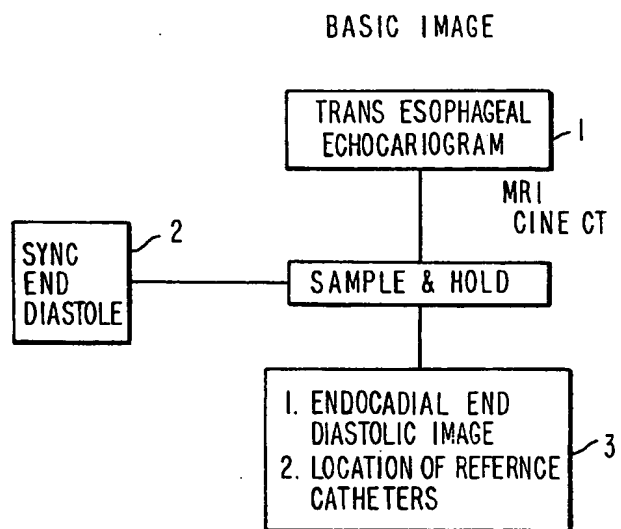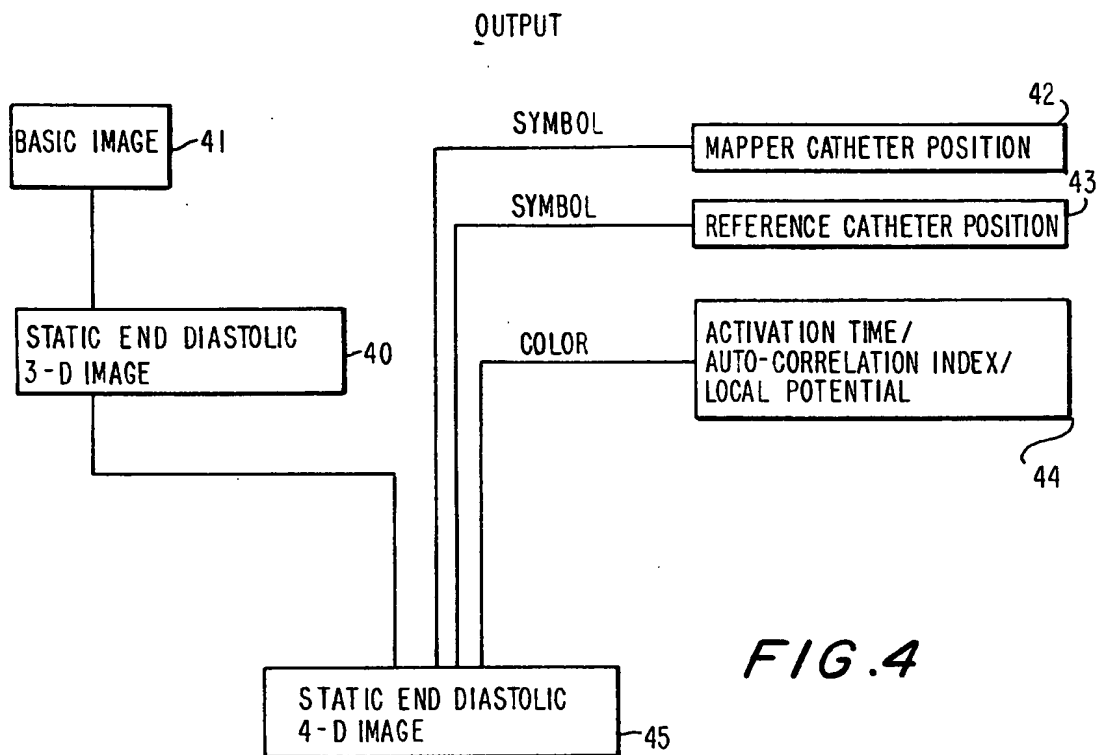*FIG. 1**FIG. 4*

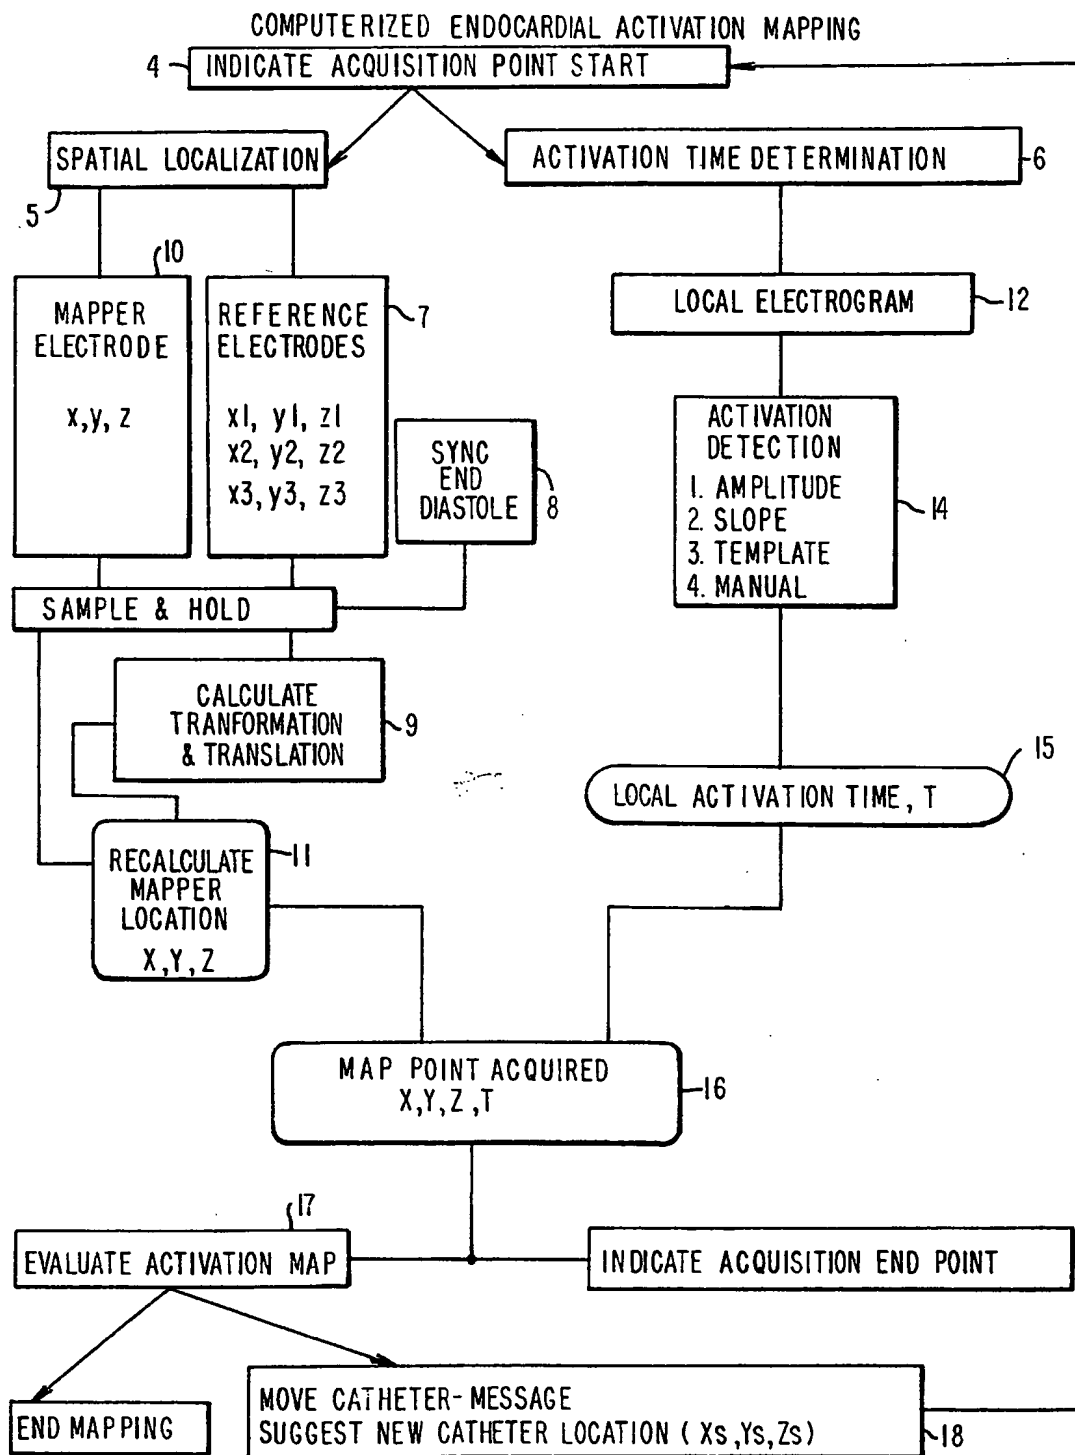
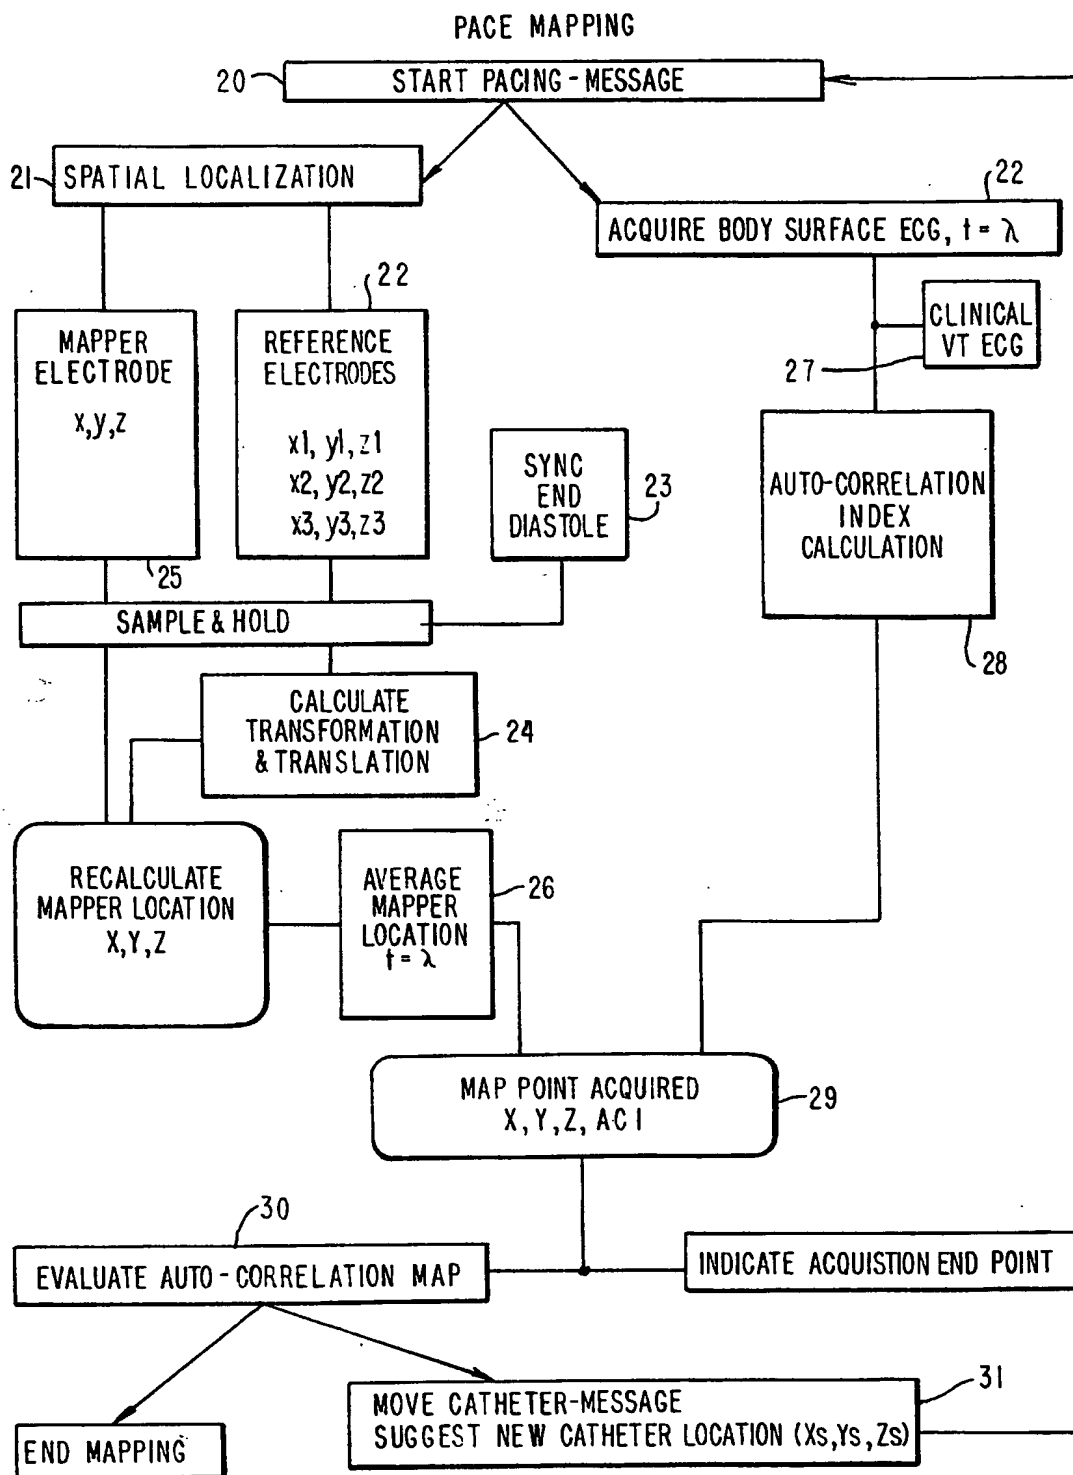
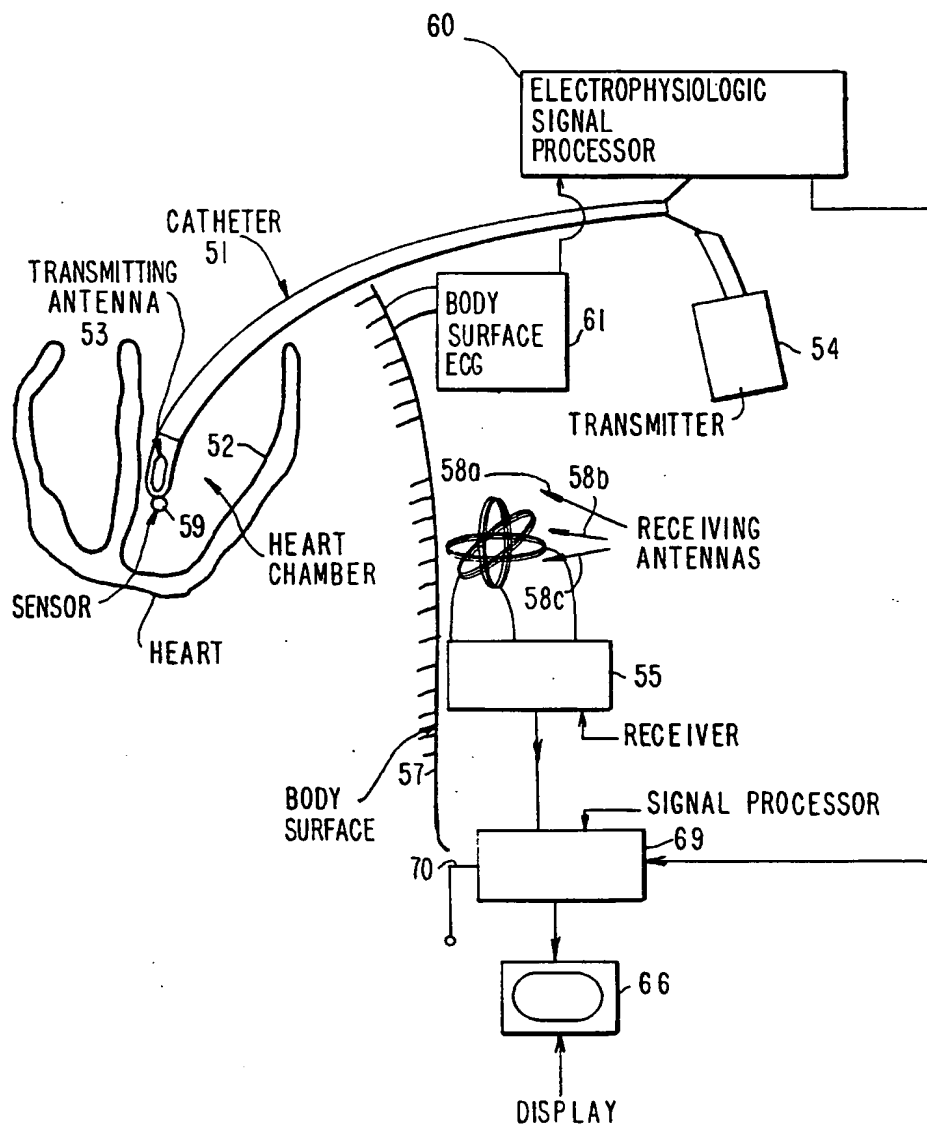
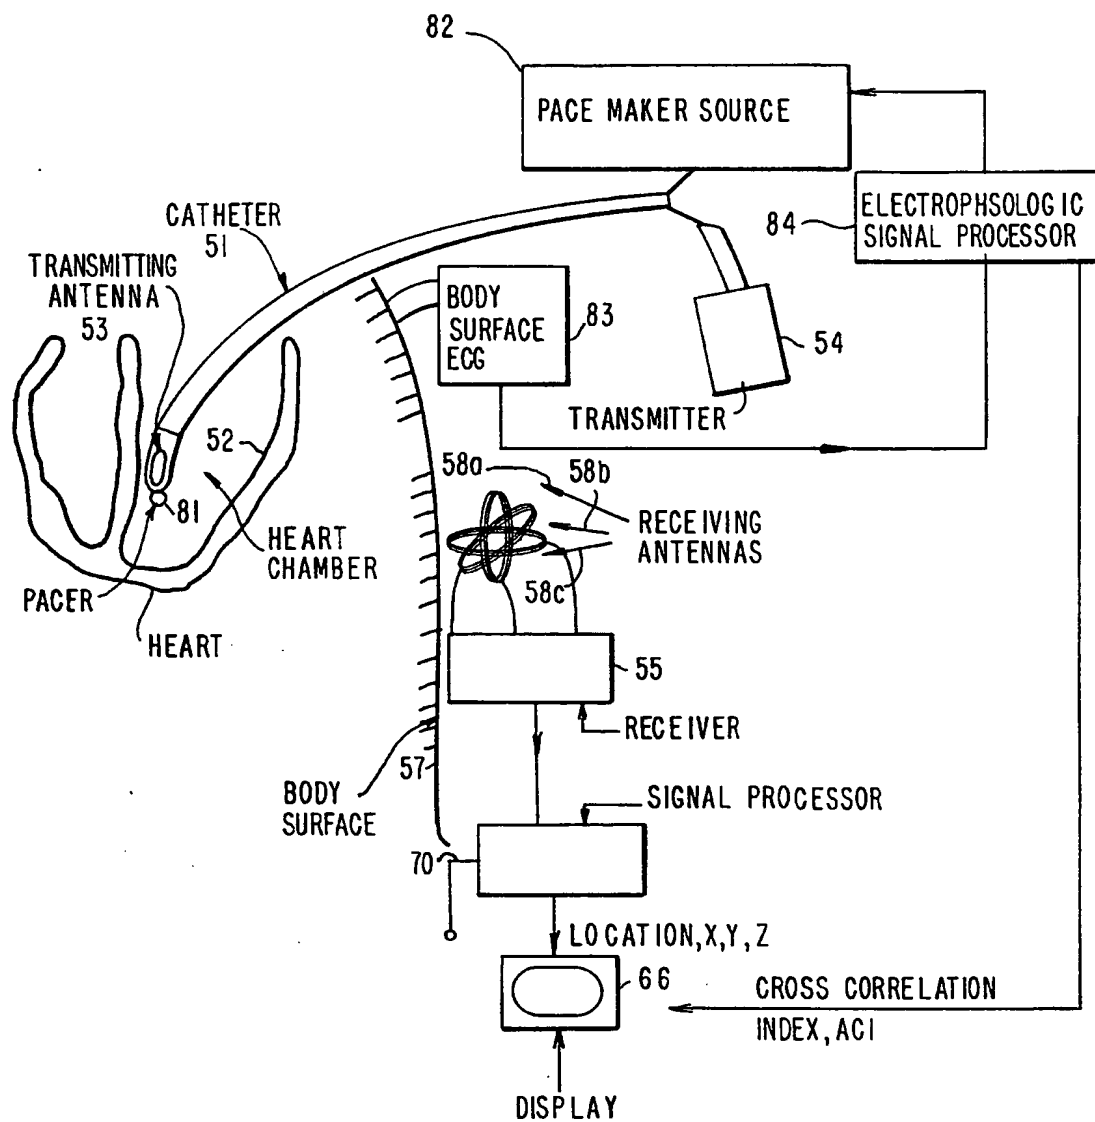
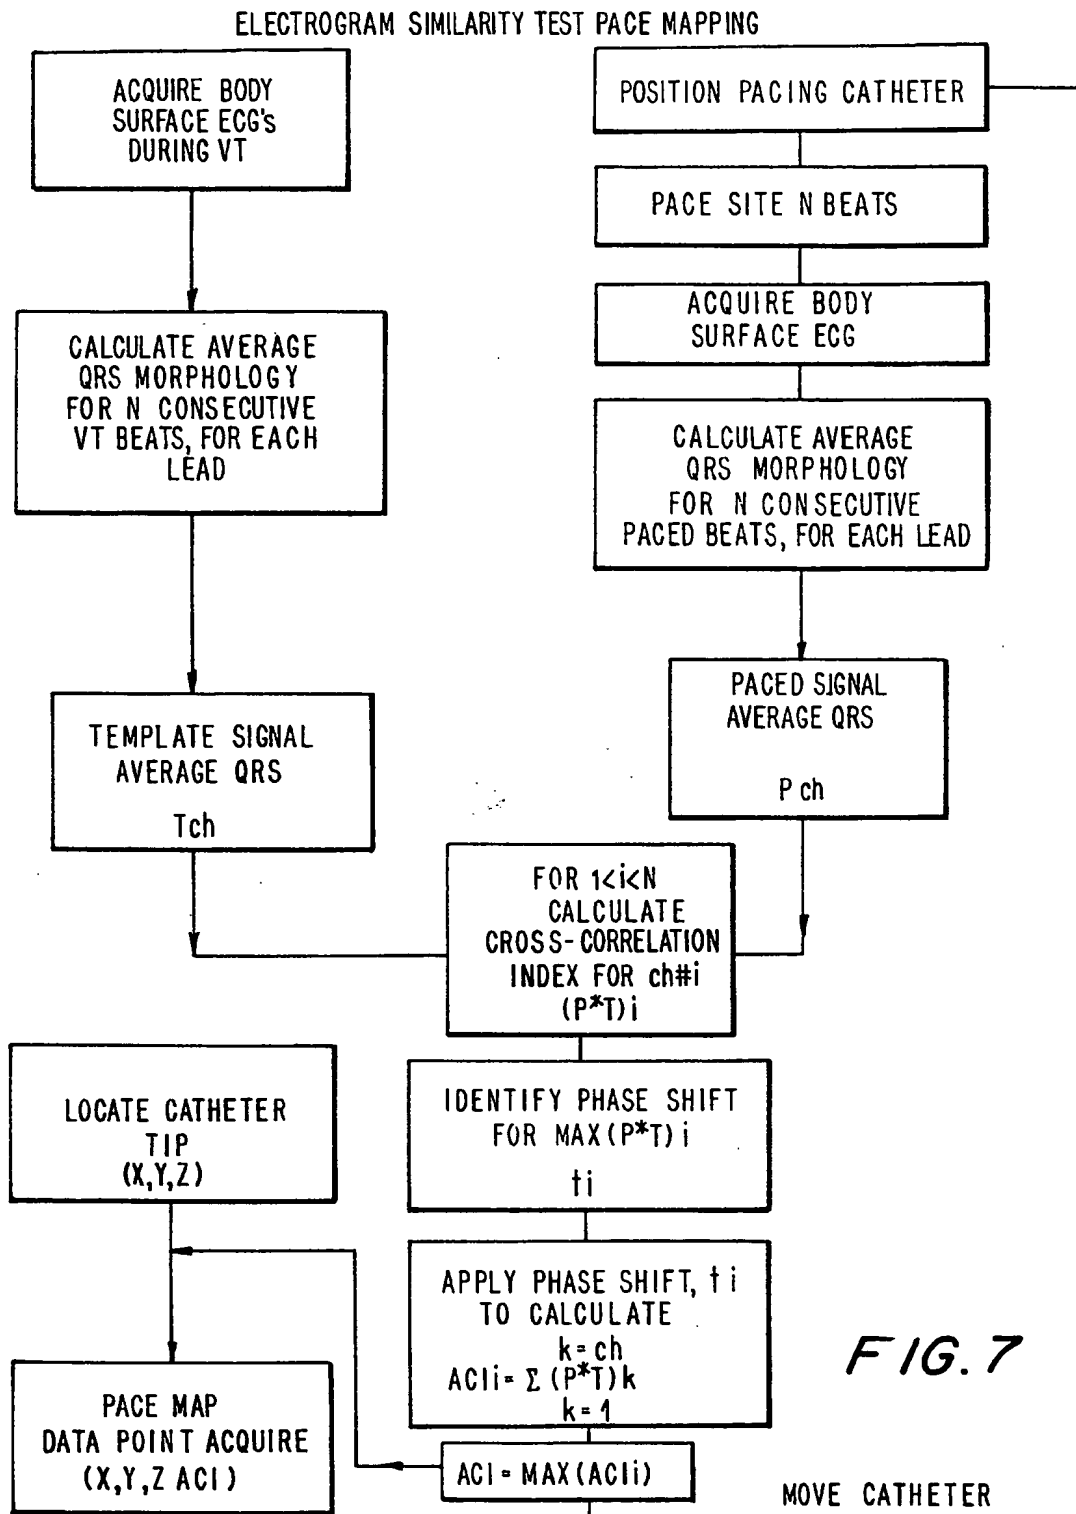


FIG. 2

**FIG. 3**

**FIG. 5**

**FIG. 6**



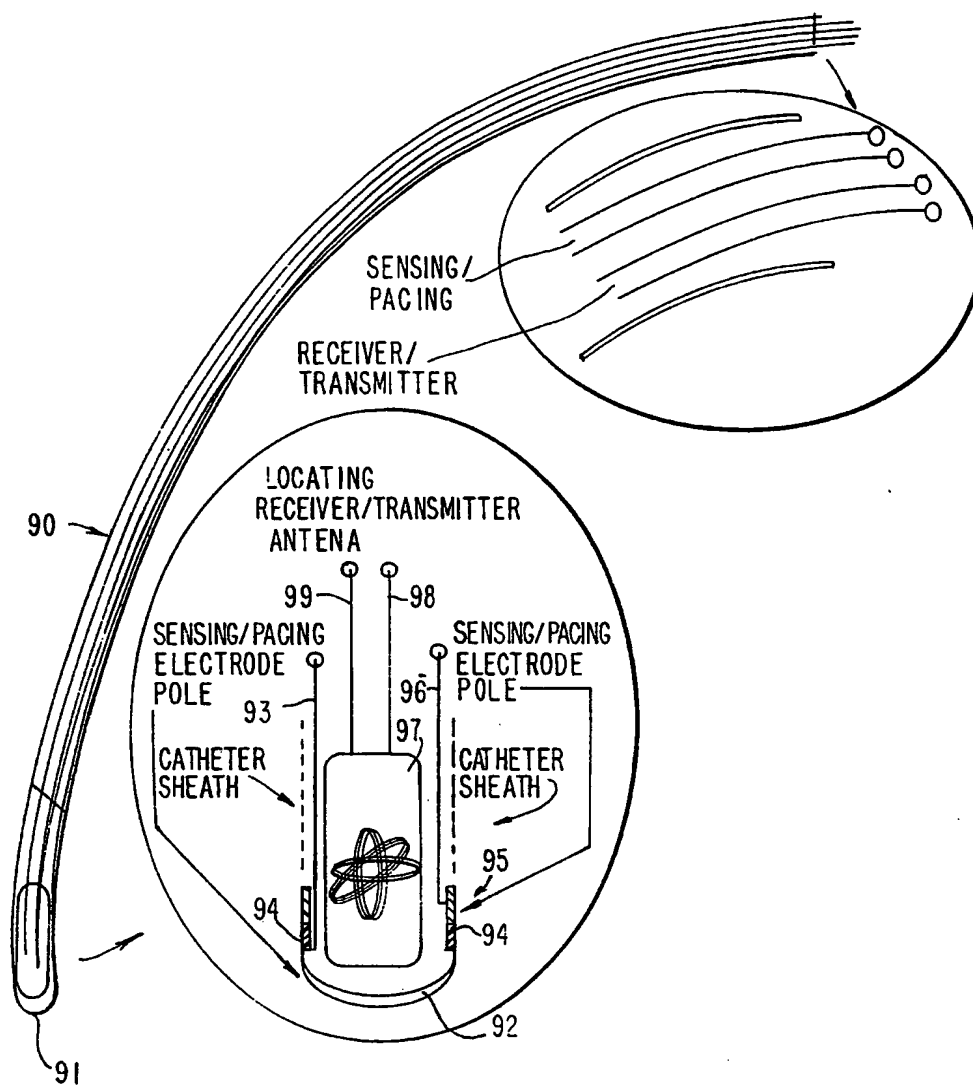


FIG. 8


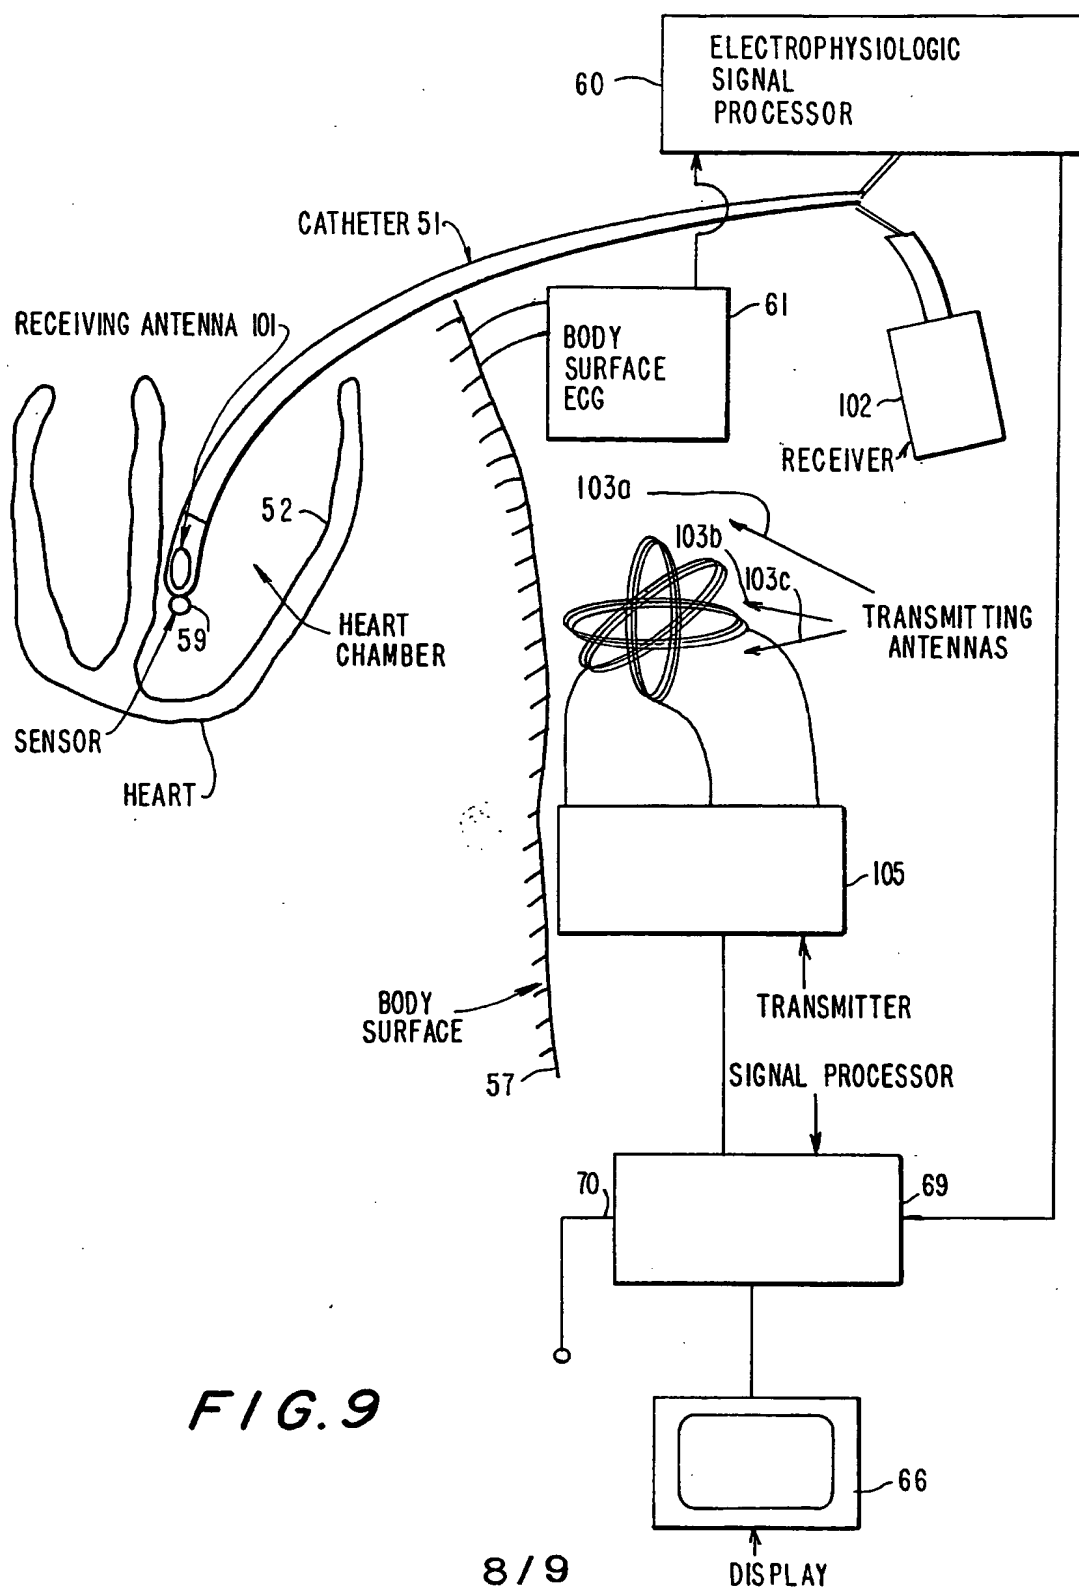


FIG. 9

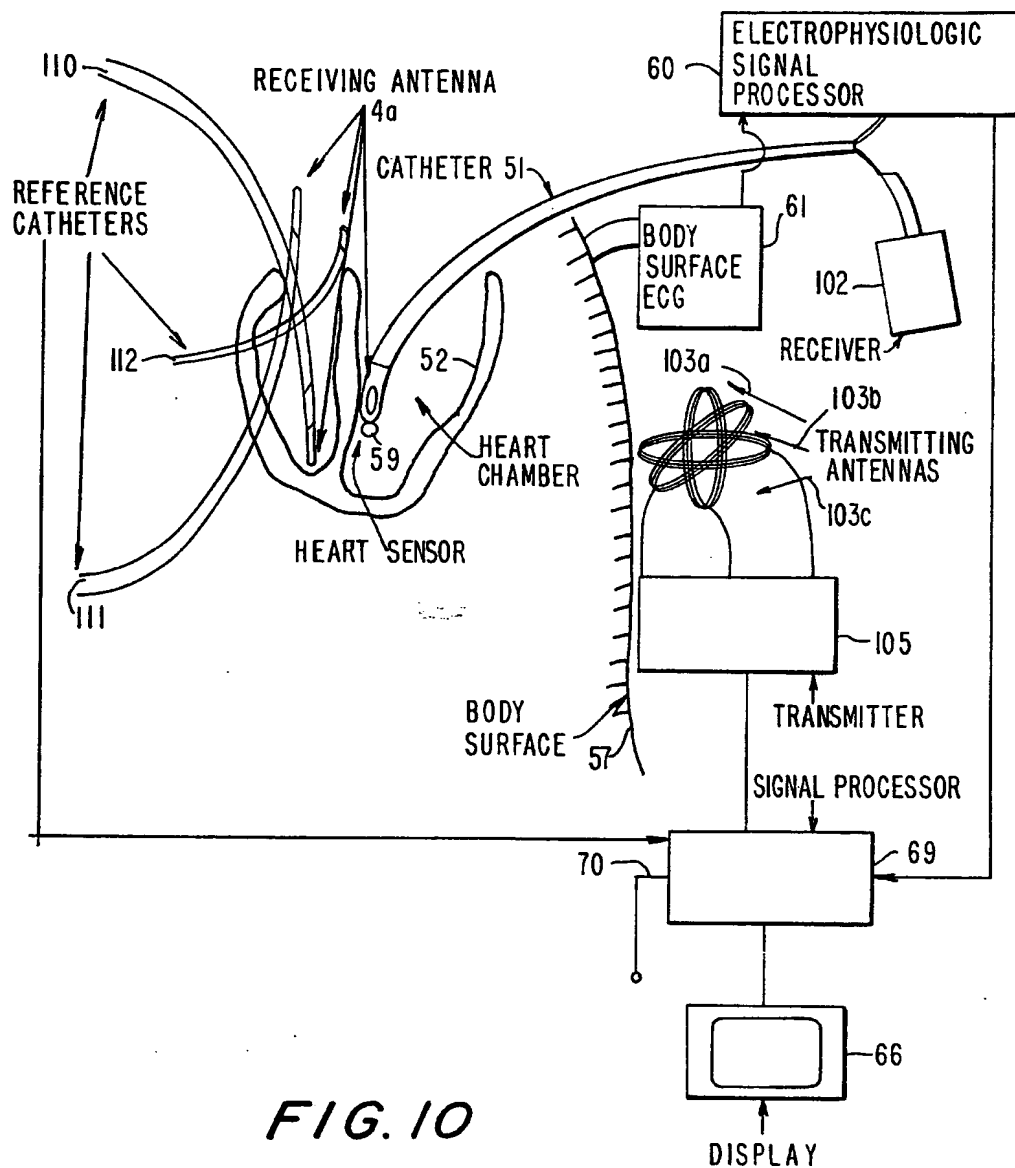

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US94/08352

A. CLASSIFICATION OF SUBJECT MATTER

IPC(5) :A61B 8/12

US CL :128/662.06

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 128/660.03, 662.06, 696, 697, 699; 607/2, 119, 122

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched
NONE

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)
NONE

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X --- Y	US, A, 5,222,501, (IDEKER ET AL.), 29 June 1993. See entire document	1-11, 13-20, 24-26, 36 i ----- 12, 22, 23, 42-44
A	US, A, 4,812,976, (LUNDY), 14 March 1989. See entire document.	27-35, 37-41
A	US, A, 5, 012,814, (MILLS ET AL.), 07 May 1991 See entire document.	27-35, 37-41

☐ Further documents are listed in the continuation of Box C. ☐ See patent family annex.

* Special categories of cited documents:	*T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
*A document defining the general state of the art which is not considered to be part of particular relevance	*X document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
*E earlier document published on or after the international filing date	*Y document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
*L document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	*A document member of the same patent family
*O document referring to an oral disclosure, use, exhibition or other means	
*P document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search

12 NOVEMBER 1994

Date of mailing of the international search report

DEC 27 1994

Name and mailing address of the ISA/US
Commissioner of Patents and Trademarks
Box PCT
Washington, D.C. 20231

Facsimile No. (703) 305-3230

Authorized officer
GEORGE MANUEL

Telephone No. (703) 308-2118